



Member State
Switzerland

OIML Certificate
No R76/2006-CH1-17.01

OIML CERTIFICATE OF CONFORMITY

Issuing authority

Name **Federal Institute of Metrologie METAS**
Conformity Evaluation Body METAS-Cert

Address Lindenweg 50, 3003 Bern-Wabern, Switzerland

Person responsible Gulian Couvreur, Head of METAS-Cert

Applicant

Name Mettler-Toledo Instruments (Shanghai) Co. Ltd.

Address Gui Ping Road 589, 200233 Shanghai, People's Republic of China

Manufacturer The manufacturer of the certified pattern is the Applicant

Identification of the certified pattern

Non-Automatic Weighing Instrument

Type **NewClassic MF**

This Certificate attests the conformity of the above identified type (represented by the sample or samples identified in the associated test report) with the requirements of the following Recommendation of the International Organization of Legal Metrology (OIML):



R 76-1, edition 2006

for accuracy class(es) **I II**

This Certificate relates only to the metrological and technical characteristics of the type of instrument covered by the relevant OIML Recommendation identified above.

This Certificate does not bestow any form of legal international approval.

OIML Certificate
No R76/2006-CH1-17.01

Metrological characteristics

Accuracy class	I	II	
		Small housing	Large housing
Max	≤ 10 200 g	120 g to 10 200 g	10 200 g to 64 200 g
e	≥ 1 mg	≥ 10 mg	≥ 1 g
d	≥ 0.01 mg	≥ 1 mg	≥ 0.1 g
n	≤ 420 000	≤ 82 000	≤ 64 200
Tare-balancing range	Until 100 % of Max		
Temperature range	10 °C / 30 °C		5 °C / 40 °C


The conformity was established by the results of tests and examinations provided in the associated Test Reports:

No / Including pages	No / Including pages	No / Including pages
511-00144 / 28	511-00361 / 28	511-01151 / 18
511-00152 / 32	511-00441 / 22	511-01177 / 7
511-00306 / 32	511-00523 / 24	
511-00339 / 18	511-00524 / 17	
511-00342 / 28	511-00525 / 17	
511-00345 / 28	511-00527 / 46	
511-00348 / 20	511-00530 / 28	
511-00351 / 17	511-01148 / 30	
511-00354 / 28	511-01149 / 30	
511-00357 / 32	511-01150 / 34	

3003 Bern-Wabern, 20 February 2017


The Issuing Authority

Federal Institute of Metrologie METAS

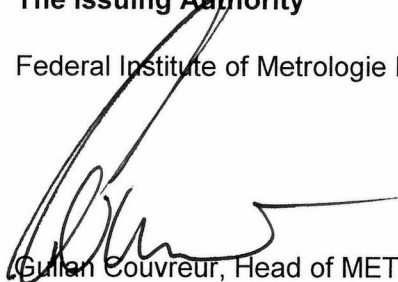

Guilan Couvreur, Head of METAS-Cert

The OIML Member



Dr. Gregor Dudle, Deputy Director

Important note: Apart from the mention of the Certificate's reference number and the name of the OIML Member State in which the Certificate is issued, partial quotation of the Certificate and the associated Test Report is not permitted, although either may be reproduced in full.