

Czech Metrology Institute





Member state **Czech Republic** OIML Certificate No. R76/2006-CZ-16.03

OIML BASIC CERTIFICATE OF CONFORMITY

Issuing Authority

Name:

Czech Metrology Institute

Address:

Okružní 31,

638 00 Brno, CZ

Person responsible: Jan Kalandra

Applicant

Name:

RADWAG WAGI ELEKTRONICZNE Witold Lewandowski

Address:

ul. Bracka 28 26-600 Radom

Poland

Manufacturer of the certified type

Name:

RADWAG WAGI ELEKTRONICZNE Witold Lewandowski

Address:

ul. Bracka 28

26-600 Radom

Poland

Identification of the certified type

Non-automatic weighing instrument

Type: PS xxx.R2.yyy

Further characteristics see pages 3 - 7.

This certificate attests the conformity of above identified type (represented by the sample (s) identified in the OIML Basic Type Evaluation Report) with the requirements of the following Recommendation of the International Organization of Legal Metrology (OIML):

OIML R 76, edition 2006 for accuracy class (II)



This certificate relates only to the metrological and technical characteristics of the type of measuring instrument covered by the relevant OIML Recommendation identified above.

This certificate does not bestow any form of legal international approval.

The conformity was established by the results of tests and examinations provided in the associated OIML Basic Type Evaluation Report(s):

No. 6051-PT-0024-13 from 29 September 2013 having 43 pages.

No. 8551-PT-E0135-13 from 23 August 2013 having 41 pages.

No. 8551-PT-E0170-13 from 12 September 2013 having 17 pages.

Certificate history:

Issue no.	Date	Description of the modification

Geskinstitus (Seskinstitus

The OIML Issuing Authority
Pavel Klenovský

12 August 2016

Important note: Apart from the mention of the Certificate's reference number and the name of the OIML Member State in which the Certificate is issued, partial quotation of the Certificate and of the associated OIML Basic Type Evaluation Report(s) is not permitted, although either may be reproduced in full.

Instrument description

Instrument PS xxx.R2.yyy model series operates on basis of electromagnetic compensation of weighed load. This series features a measuring range up to 6000g. Instrument has LCD display, plastic cover, stainless steel plate, automatic internal adjustment system. Symbol xxx stands for Max (g) and symbol yyy stands for special purpose of balance e.g. jewelry balance – CT.

Description of the instrument:

Description	Drawing number	
Schedule of balance working	PS.R2-01-010	
Side view	PS.R2 -10-1000 sheet 2/3 and PS.R2 -10-6000 sheet 2/3	
Localization of nominal label	PS.R2 -10-1010	
Display	PS.R2-20-000	
Data plate	PS.R2- 90- 400	
View with open case	PS.R -10-1000 sheet 3/3 and PS.R -10-6000 sheet 3/3	
PCB	PCB 365	

Metrological characteristic

Type	PS	PS	PS	PS	PS		
	200/2000.R2	250.R2	1000.R2	1500.R2	6000.R2		
Maximum - Max	200/2000 g	250 g	1000 g	1500 g	6000 g		
Minimum - Min	20/500 mg	20	mg	500 mg			
Resolution – d	1/10 mg	1 mg		10 mg			
Verification interval – e	10/100 mg	10 mg		100 mg			
Tare range – T	-200/-2000 g	-250 g	-1000 g	-1500 g	-6000 g		
Working temperature	+10 °C / +40 °C						
Supply	100 V – 240 VAC, 50-60 Hz / 12 – 16 VDC						
Accuracy class							

The above table is an example of some models within the approved range.

Characteristics and devices

The instruments must be equipped with a level indicator with a sensitivity of at least 2 mm for a tilt of 2/1000.

Devices:

- Zero indicator
- Stability indicator
- Internal adjustment
- · Service menu via switch on the main board
- Initial zero-setting
- Zero-tracking
- Data Storage Device (Alibi memory)
- Weighing in carat units*)

^{*)} For instruments that are able to display in both units if the Max, Min and e values are on a label then they must be marked on the instrument in both units. If the values are shown on a display, then they can be switched.

Data Storage Device (Alibi memory)

Models of PS xxx.R2.yyy balances are equipped with a Data Storage Device (Alibi memory) acting as a long term memory. It automatically saves weighing results according to principles of WELMEC 2.5 in the internal flash memory. A program operates as a simple embedded software without any operating system which prevents from running any external application. The program allows to upload the content of the alibi memory to an external flash drive for archival purposes. The program does not allow to download the alibi memory content to the balance. Each measurement is identified by the following data:

- Measurement date
- Measurement time
- Measurement value (mass)
- Tare value
- Operator (if logged on)
- Product (if chosen)

The memory size allows to save 100 000 weighing results. After the full capacity is reached the single records of the oldest data are overwritten by new data. Single records and the whole database are protected by checksums. Any corruption of data prevents them from viewing or printing.

Interfaces

Interfaces used must comply with 5.3.6 of OIML R76 (2006). Following interface is used: RS 232, USB 2.0. Optionally the balances may be equipped in wireless interfaces WiFi or BlueTooth.

Software

Instruments are equipped with embedded software that is used in a fixed hardware and software environment and cannot be modified or uploaded via any interface or by other means after securing and/or verification. Software identification by its version number is accessible after pressing ON/OFF key on the overlay.

The valid software version is: 4.0.0


Connectable devices

For applications not subject to mandatory verification, any peripheral devices may be connected.

Drawing 1 - Side view:



Drawing 2 - Main label position and sealing scheme:

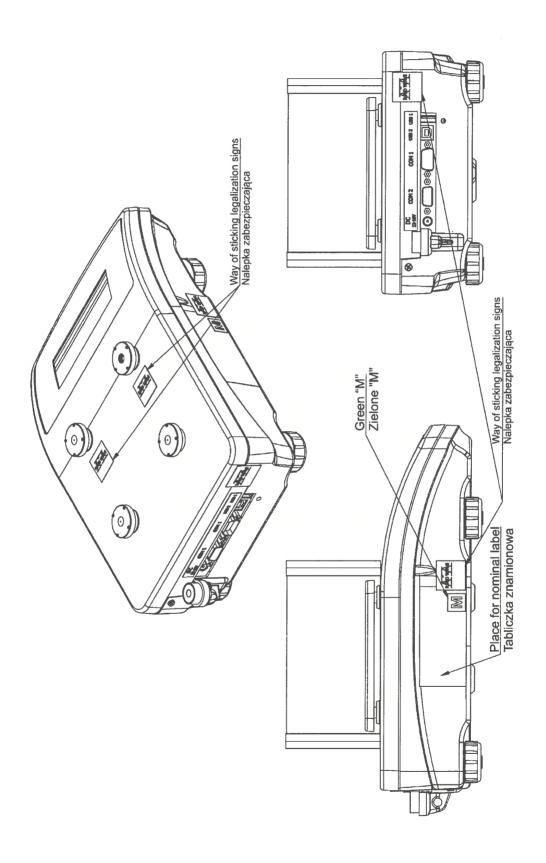

Drawing 3 – Overlay with display:

