

OIML Member State
The Netherlands

Number R76/2006-NL1-11.15 revision 1
Project number SO16200211
Page 1 of 2

Issuing authority	NMi Certin B.V. Person responsible: C. Oosterman
Applicant and Manufacturer	Ohaus Corporation 7 Campus Drive, Suite 310 Parsippany, NJ 07054 United States of America
Identification of the certified type	A Non-automatic weighing instrument Type : Navigator NV series Valor 1500 V15P series
Characteristics	See next page


This Certificate attests the conformity of the above identified Type (represented by the sample(s) identified in the OIML Test Report) with the requirements of the following Recommendation of the International Organization of Legal Metrology (OIML):

OIML R 76 - Edition 2006 for accuracy class **III**

This Certificate relates only to the metrological and technical characteristics of the type of measuring instrument covered by the relevant OIML International Recommendation above-identified.
This Certificate does not bestow any form of legal international approval.

Important note: Apart from the mention of the Certificate's reference number and the name of the OIML Member State in which the Certificate was issued, partial quotation of the Certificate and of the associated OIML Test Report(s) is not permitted, although either may be reproduced in full.

Issuing Authority **NMi Certin B.V., OIML Issuing Authority NL1**
17 March 2016

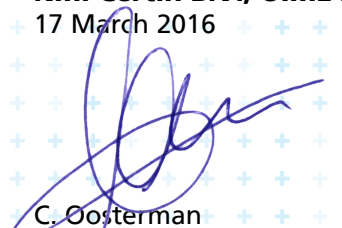

C. Oosterman
Head Certification Board

NMi Certin B.V.
Hugo de Grootplein 1
3314 EG Dordrecht
the Netherlands
T +31 78 6332332
certin@nmi.nl
www.nmi.nl

This document is issued under the provision that no liability is accepted and that the applicant shall indemnify third-party liability.

The notification of NMi Certin B.V. as Issuing Authority can be verified at www.oiml.org

Parties concerned can lodge objection against this decision, within six weeks after the date of submission, to the general manager of NMi (see www.nmi.nl).



The conformity was established by the results of tests and examinations provided in the associated OIML Test Report(s):

- Number NMI-10200718-01 dated 7 February 2011 that includes 56 pages;
- Number NMI-10200718-02 dated 7 February 2011 that includes 43 pages;
- Number NMI-11200306-01 dated 25 May 2011 that includes 28 pages.

Characteristics of the non-automatic weighing instrument:

Accuracy class	III
Maximum capacity	0,310 kg ≤ Max ≤ 16 kg or 1550 ct ≤ Max ≤ 80000 ct
Verification scale interval	e ≥ 0,1 g or e ≥ 0,5 ct
Weighing range(s)	Single-interval
Maximum number of scale intervals (one weighing range)	n ≤ 3200 divisions
Tare	T ≤ -Max
Temperature range	0 °C / 40 °C
Power supply voltage	100 - 240 V AC, 50/60 Hz adapter with 9 V DC to 12 V DC output 4 x 1,5 V DC batteries 6 V DC rechargeable battery

Revision History

This revision replaces the previous version.

Revision	Date	Change(s)
Initial	7 June 2011	-
1	17 March 2016	Added new type designation Valor 1500 V15P series.