

**OIML Member State**  
The Netherlands

Number R76/2006-A-NL1-18.24  
Project number 1902007  
Page 1 of 2

Issuing authority	NMi Certin B.V. Person responsible: C. Oosterman
Applicant and Manufacturer	Ohaus Corporation 7 Campus Drive, Suite 310 Parsippany, NJ 07054 United States of America
Identification of the certified type	A <b>Non-automatic weighing instrument</b> Type : PJX..., PR..., PX..., PXP...
Characteristics	See next page

This OIML Certificate is issued under scheme A.


This Certificate attests the conformity of the above identified Type (represented by the sample(s) identified in the OIML Test Report) with the requirements of the following Recommendation of the International Organization of Legal Metrology (OIML):

**OIML R 76** - Edition 2006 for accuracy class **I** or **II**

This Certificate relates only to the metrological and technical characteristics of the type of measuring instrument covered by the relevant OIML International Recommendation above-identified.  
This Certificate does not bestow any form of legal international approval.

*Important note:* Apart from the mention of the Certificate's reference number and the name of the OIML Member State in which the Certificate was issued, partial quotation of the Certificate and of the associated OIML Test Report(s) is not permitted, although either may be reproduced in full.

Issuing Authority **NMi Certin B.V., OIML Issuing Authority NL1**  
4 June 2018

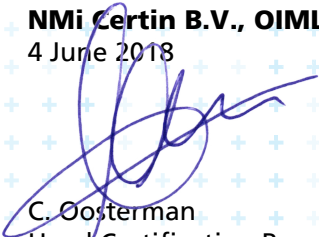

C. Oosterman  
Head Certification Board

NMi Certin B.V.  
Hugo de Grootplein 1  
3314 EG Dordrecht  
the Netherlands  
T +31 78 6332332  
certin@nmi.nl  
www.nmi.nl

This document is issued under the provision that no liability is accepted and that the applicant shall indemnify third-party liability.

The notification of NMi Certin B.V. as Issuing Authority can be verified at [www.oiml.org](http://www.oiml.org)



**OIML Member State**  
The Netherlands

Number R76/2006-A-NL1-18.24  
Project number 1902007  
Page 2 of 2

The conformity was established by the results of tests and examinations provided in the associated OIML Test Reports:

- No. NMI-1902007-01 dated 29 May 2018 that includes 33 pages;
- No. NMI-1902007-02 dated 29 May 2018 that includes 28 pages.
- No. NMI-1902007-03 dated 29 May 2018 that includes 35 pages;
- No. NMI-1902007-04 dated 29 May 2018 that includes 31 pages;
- No. NMI-1902007-05 dated 29 May 2018 that includes 28 pages.

**Characteristics of the non-automatic weighing instrument:**

Accuracy class	Ⓘ	Ⓜ
Maximum capacity	Max ≤ 240 g or Max ≤ 1200 ct	Max ≤ 8200 g or Max ≤ 41000 ct
Verification scale interval	e ≥ 0,001 g or 0,005 ct	e ≥ 0,01 g or 0,05 ct
Actual scale interval	e = d, e = 10 d, or e = 100 d	e = d, or e = 10 d
Weighing range	Single interval	
Maximum number of scale intervals	n ≤ 240000 divisions	n ≤ 62000 divisions
Tare	T ≤ -Max	
Temperature range	+15 °C / +25 °C (*) or +10 °C / +30 °C	+10 °C / +30 °C
Power supply voltage	12 V DC supplied by a 100 – 240 V AC 50/60 Hz adapter	
Software identification	Version number 1.xx (xx is a number between 01 and 99) (1 represents the legally relevant software)	

(\*) for models PX...5...