

**OIML Member State**  
The Netherlands

Number R76/2006-A-NL1-18.29  
Project number 1902209  
Page 1 of 2

Issuing authority NMI Certin B.V.  
Person responsible: C. Oosterman

Manufacturer Charder Electronic Co Ltd  
No. 103, Guozhong Rd., Dali Dist.  
Taichung City 412,  
Taiwan (R.O.C.)

Identification of the certified type **A Non-automatic weighing instrument**  
Type : MS7800

Characteristics See next page

This OIML Certificate is issued under scheme A.


This Certificate attests the conformity of the above identified Type (represented by the sample(s) identified in the OIML Test Report) with the requirements of the following Recommendation of the International Organization of Legal Metrology (OIML):

**OIML R 76** - Edition 2006 for accuracy class **III**

This Certificate relates only to the metrological and technical characteristics of the type of measuring instrument covered by the relevant OIML International Recommendation above-identified.  
This Certificate does not bestow any form of legal international approval.

*Important note:* Apart from the mention of the Certificate's reference number and the name of the OIML Member State in which the Certificate was issued, partial quotation of the Certificate and of the associated OIML Test Report(s) is not permitted, although either may be reproduced in full.

Issuing Authority **NMI Certin B.V., OIML Issuing Authority NL1**  
17 September 2018

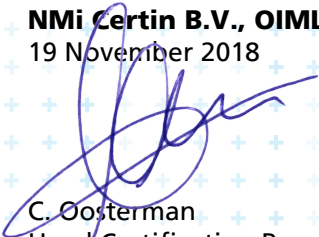

C. Oosterman  
Head Certification Board

NMI Certin B.V.  
Hugo de Grootplein 1  
3314 EG Dordrecht  
the Netherlands  
T +31 78 6332332  
certin@nmi.nl  
www.nmi.nl

This document is issued under the provision that no liability is accepted and that the applicant shall indemnify third-party liability.

The notification of NMI Certin B.V. as Issuing Authority can be verified at [www.oiml.org](http://www.oiml.org)



**OIML Member State**  
The Netherlands

Number R76/2006-A-NL1-18.29  
Project number 1902209  
Page 2 of 2

The conformity was established by the results of tests and examinations provided in the associated OIML Type Evaluation Report(s):

- No. NMI-1902209-02 dated 17 September 2018 that includes 43 pages.

**Characteristics of the non-automatic weighing instrument:**

Accuracy class	(III)
Maximum capacity	Max $\leq$ 250 Kg
Verification scale interval	e $\geq$ 0,5 Kg
Weighing range(s)	Single interval
Maximum number of scale intervals	n $\leq$ 500 divisions
Temperature range	+ 5 °C / + 35 °C
Power supply voltage	3,7 V DC by the battery
Application	To be used only for weighing patients
Software identification	Version number
	P1.xx (xx = 00 ~ 99)