

**OIML Member State**  
The Netherlands

Number R76/2006-A-NL1-18.35  
Project number 1902117  
Page 1 of 2

Issuing authority NMI Certin B.V.  
Person responsible: C. Oosterman

Applicant and Manufacturer Hill-Rom, Inc.  
1069 State Route 46 East  
Batesville, IN 47006  
United States of America

Identification of the certified type **A Non-automatic weighing instrument**  
Type : Centrella

Characteristics See next page

This OIML Certificate is issued under scheme A.


This Certificate attests the conformity of the above identified Type (represented by the sample(s) identified in the OIML Test Report) with the requirements of the following Recommendation of the International Organization of Legal Metrology (OIML):

**OIML R 76** - Edition 2006 for accuracy class  $\textcircled{\text{III}}$  or  $\textcircled{\text{III}}$

This Certificate relates only to the metrological and technical characteristics of the type of measuring instrument covered by the relevant OIML International Recommendation above-identified.  
This Certificate does not bestow any form of legal international approval.

*Important note:* Apart from the mention of the Certificate's reference number and the name of the OIML Member State in which the Certificate was issued, partial quotation of the Certificate and of the associated OIML Test Report(s) is not permitted, although either may be reproduced in full.

Issuing Authority **NMI Certin B.V., OIML Issuing Authority NL1**  
16 October 2018

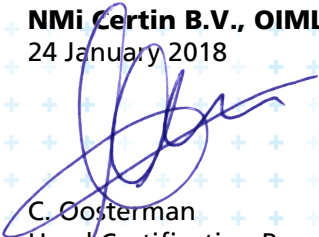

C. Oosterman  
Head Certification Board

NMI Certin B.V.  
Hugo de Grootplein 1  
3314 EG Dordrecht  
the Netherlands  
T +31 78 6332332  
certin@nmi.nl  
www.nmi.nl

This document is issued under the provision that no liability is accepted and that the applicant shall indemnify third-party liability.

The notification of NMI Certin B.V. as Issuing Authority can be verified at [www.oiml.org](http://www.oiml.org)



**OIML Member State**  
The Netherlands

Number R76/2006-A-NL1-18.35  
Project number 1902117  
Page 2 of 2

The conformity was established by the results of tests and examinations provided in the associated OIML Type Evaluation Report(s):

- No. NMI-1902117-01 dated 16 October 2018 that includes 50 pages.

**Characteristics of the non-automatic weighing instrument:**

Accuracy class	III or IIII
Maximum capacity	Max $\leq$ 250 kg
Verification scale interval	$e \geq$ 0,5 kg
Weighing range(s)	Single interval
Maximum number of scale intervals (one weighing range)	$n \leq$ 500 divisions
Temperature range	+5 °C / +35 °C
Power supply voltage	100 - 240 V AC 50/60 Hz
Application	Intended to be used for weighing patients
Software identification	V2