



| | | |
|--|---|--|
|  |  |  |
| OIML Member State Denmark | | OIML Certificate No. R76/2006-A-DK2-25.02 |
| OIML CERTIFICATE ISSUED UNDER SCHEME A | | |
| OIML Issuing Authority Name: FORCE Certification A/S Address: Park Allé 345, 2605 Brøndby, Denmark Person responsible: Per Rafn Crety | | |
| Applicant Name: A.A Eliyahu (Odaya) Cashmal Ltd, Address: Yosef Sapir 6, Rishon Le-Zion, Israel | | |
| Manufacturer A.A Eliyahu (Odaya) Cashmal Ltd. | | |
| Identification of the certified type <i>(the detailed characteristics will be defined in the additional pages)</i> ACS-268 | | |
| Designation of the module <i>(if applicable)</i> Non-automatic weighing instrument | | |
| <p>This OIML Certificate attests the conformity of the above identified type (represented by the sample(s) identified in the OIML type evaluation report) with the requirements of the following Recommendation of the International Organization of Legal Metrology (OIML):</p> <p>OIML R 76-1, Edition (year): 2006</p> <p>For accuracy class (if applicable): III</p> | | |

This OIML Certificate relates only to metrological and technical characteristics of the type of measuring instrument covered by the relevant OIML Recommendation identified above.

This OIML Certificate does not bestow any form of legal international approval.

The conformity was established by the results of tests and examinations provided in the associated OIML reports:

Type examination report:

DANAK-1913671, dated 12 December 2014, that includes 68 pages

DANAK-1914393, dated 12 August 2014, that includes 20 pages

121-25987.10, dated 02 November that includes 26 pages.

Type evaluation report: No. 124-34592.90.10, dated 15 January 2025, that includes 21 pages

The technical documentation relating to the identified type is contained in documentation file:
T207529 and 121-25987

OIML Certificate History

| Revision No. | Date | Description of the modification |
|-----------------|---------------|---------------------------------|
| Initial version | 22 April 2025 | - |
| | | |
| | | |
| | | |

Identification, signature and stamp

The OIML Issuing Authority

FORCE Certification A/S

Date: 22 April 2025

Jens Hovgård Jensen

Certification Manager

Important note: Apart from the mention of the Certificate's reference number and the name of the OIML Member State in which the Certificate is issued, partial quotation of the Certificate and of the associated OIML type evaluation report(s) is not permitted, although either may be reproduced in full.

Descriptive annex

Characteristics

| | | |
|-------------------------------------|----------------------|--|
| Accuracy class | | III |
| Weighing range | | Single-interval or dual-range |
| Maximum capacity | Max | 3 kg to 30 kg |
| Minimum capacity | Min | 20 e |
| Verification scale interval | e | ≥ 1 g |
| Number of intervals | Max_i / e_i | ≤ 3000 |
| Subtractive tare | T | $\leq -\text{Max}$ |
| Interface | | None |
| Supply voltage | | 220 VAC, 50 Hz, optional internal battery |
| Temperature range for the indicator | | -10 °C / +40 °C |
| Software identification: | | 120305 |

Devices

- Initial zero setting $\leq \pm 10\%$ of Max.
- Semi-automatic zero-setting $\leq \pm 2\%$ of Max
- Zero-tracking $\leq \pm 2\%$ of Max
- Semi-automatic tare
- Price look-up (M1 to M8)

Software


The software revision level is displayed during the power-up sequence of the instrument.

The approved software version is 210906

EMC protection

For the models with 220 VAC power supply shall a number of ferrites and line filters be mounted inside the scale.

The presence and position of the components shall be checked at verification.

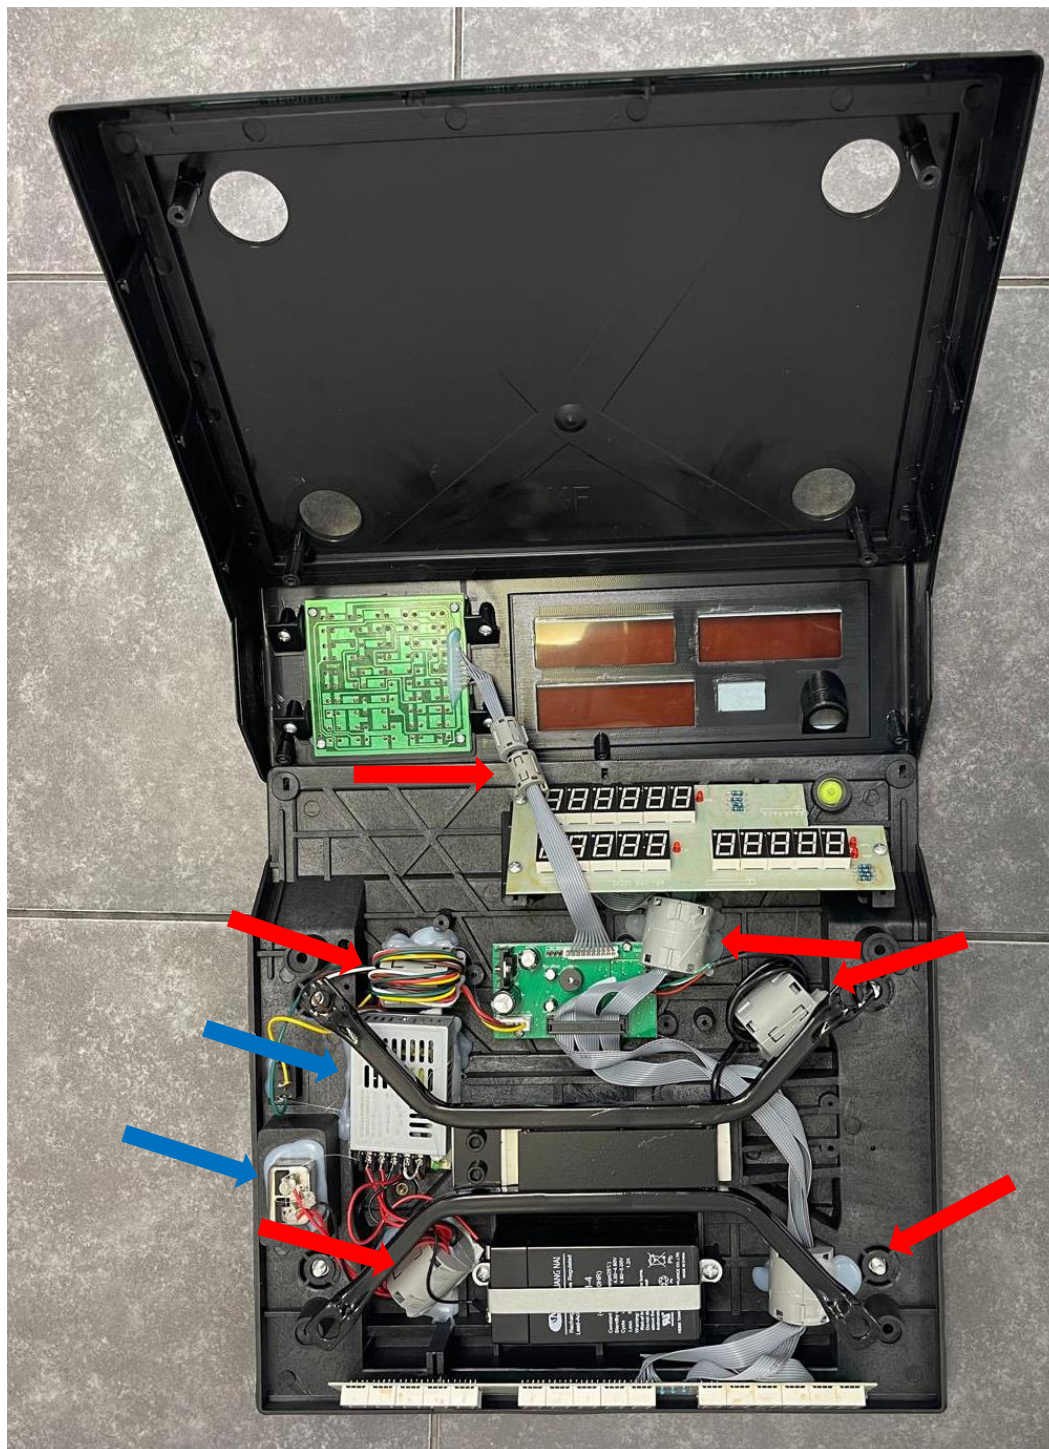

Ferrites position

Line filter position

